

FIGURE 1A

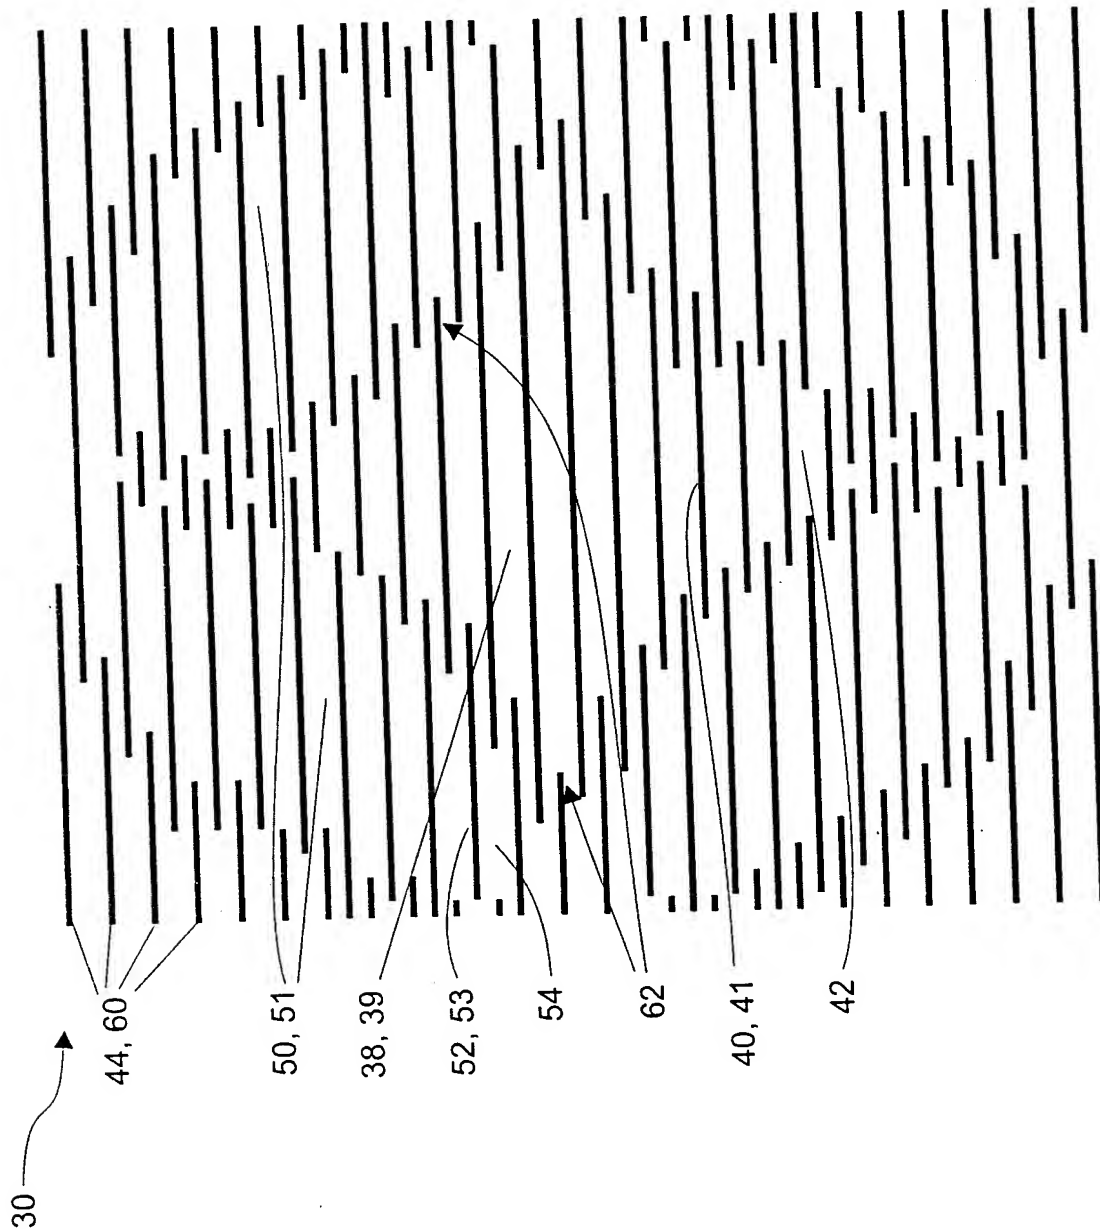


FIGURE 1A

FIGURE 1B

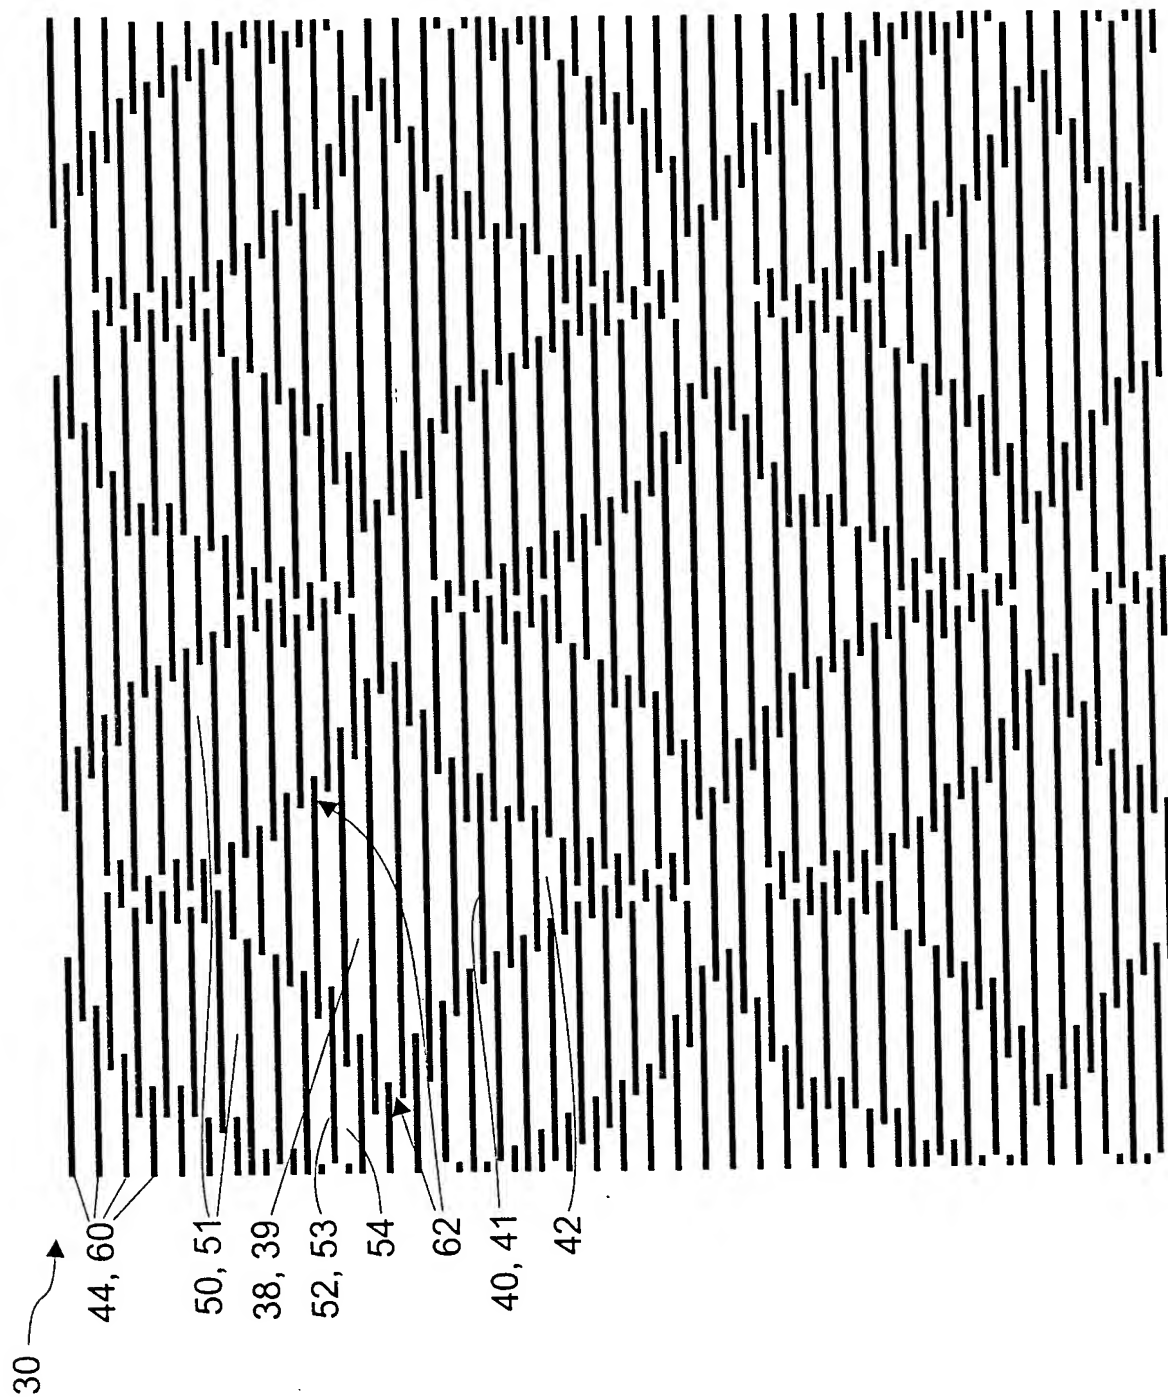


FIGURE 1B

FIGURE 2

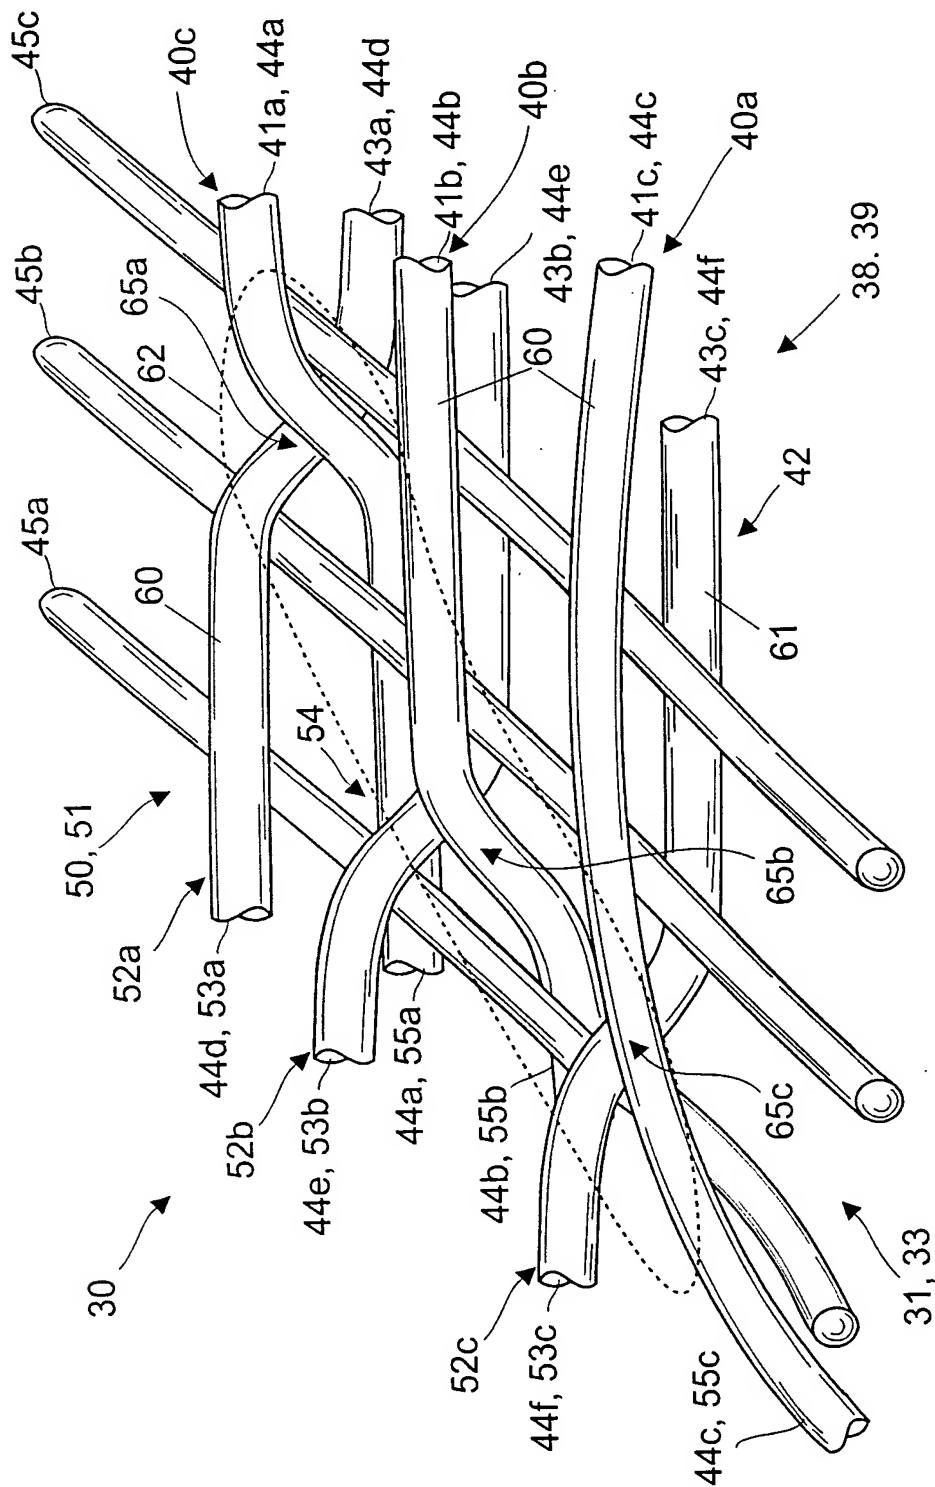


FIGURE 2

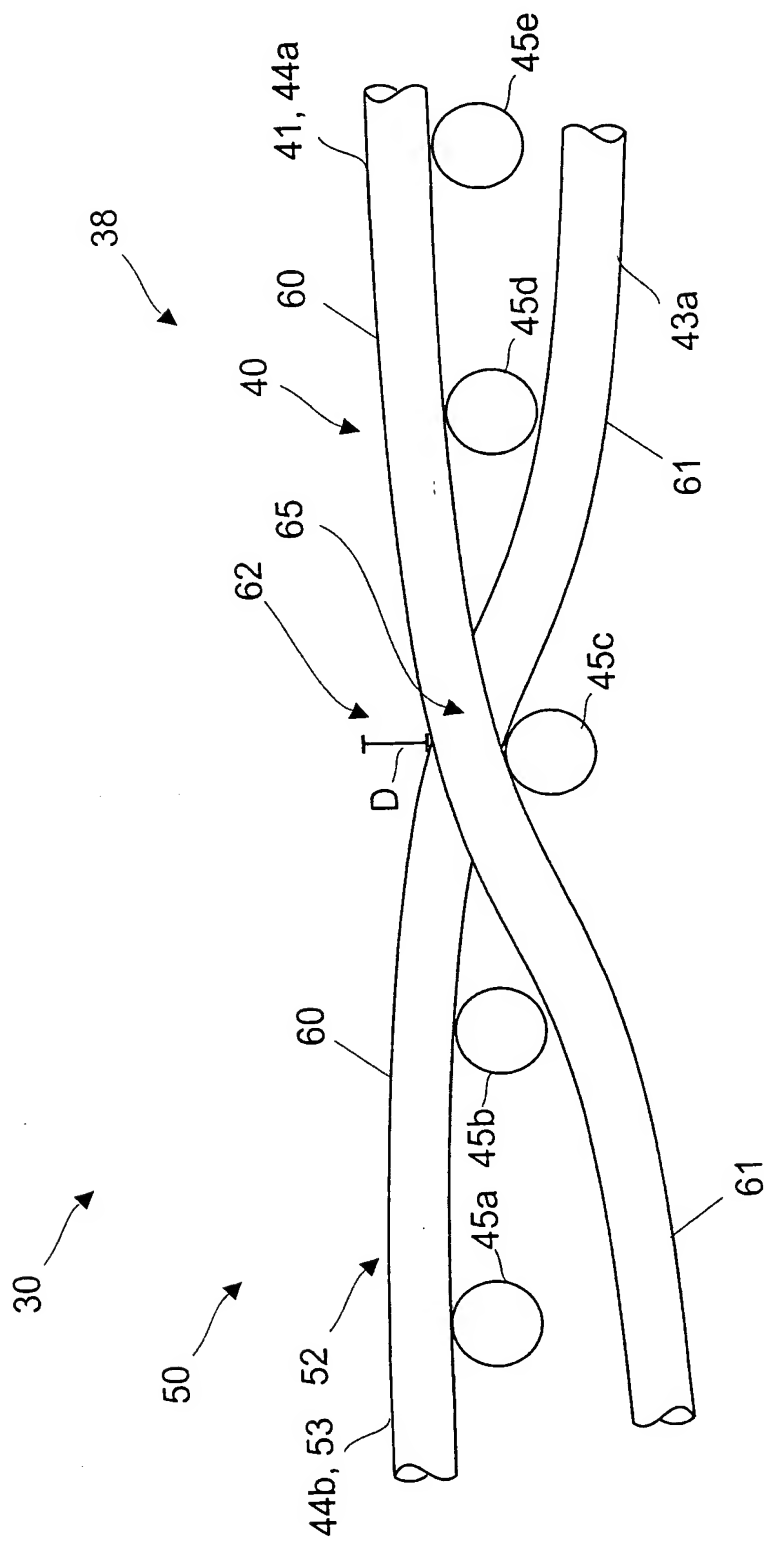


FIGURE 3

FIG. 4

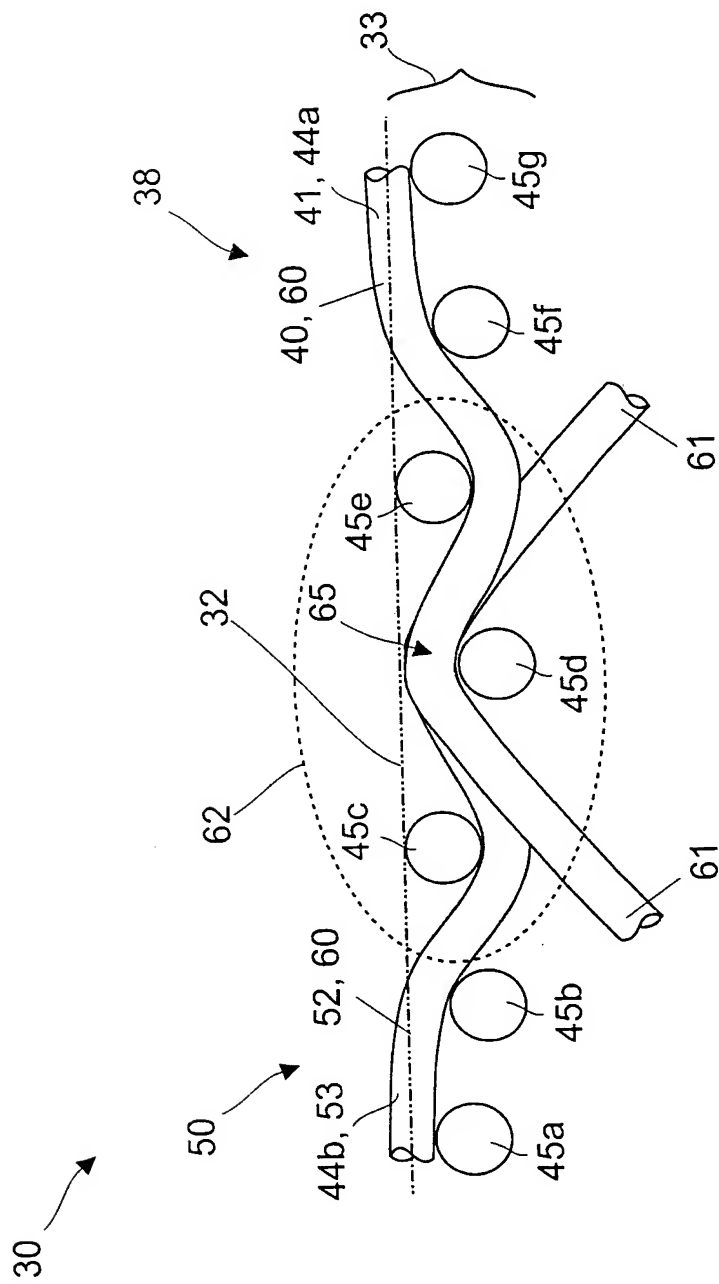


FIGURE 4

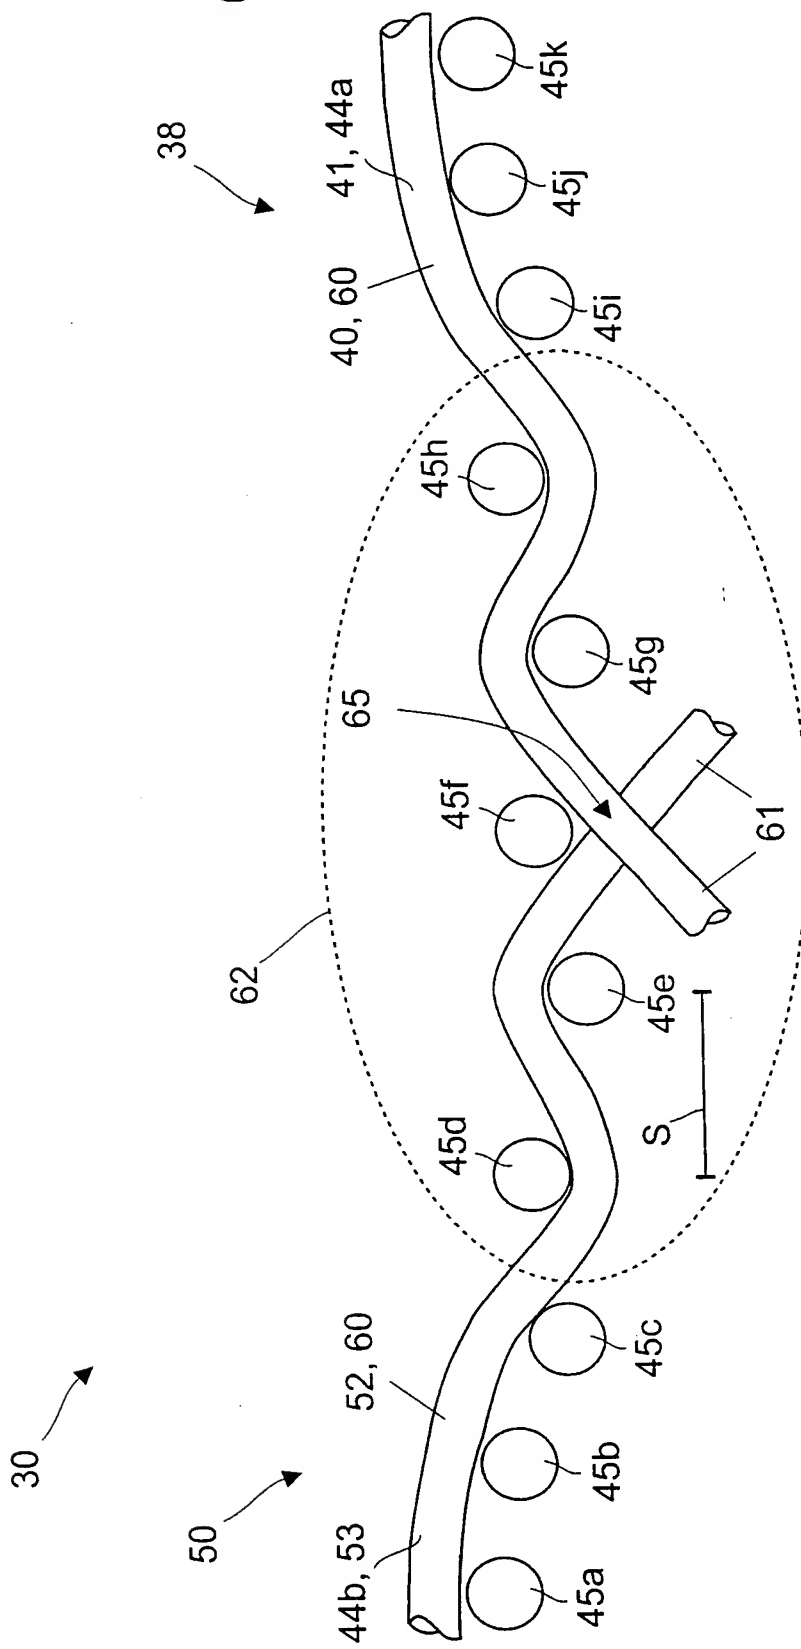


FIGURE 5

Figure 1. The effect of the number of trials on the number of correct responses. The number of correct responses was significantly higher than the number of incorrect responses in all cases.



FIGURE 6

FIG. 7

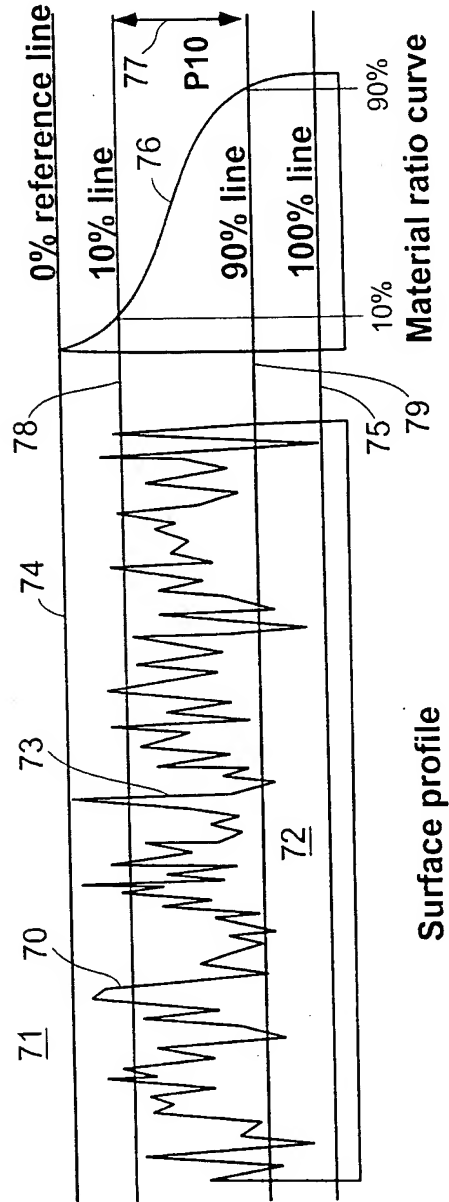


FIGURE 7

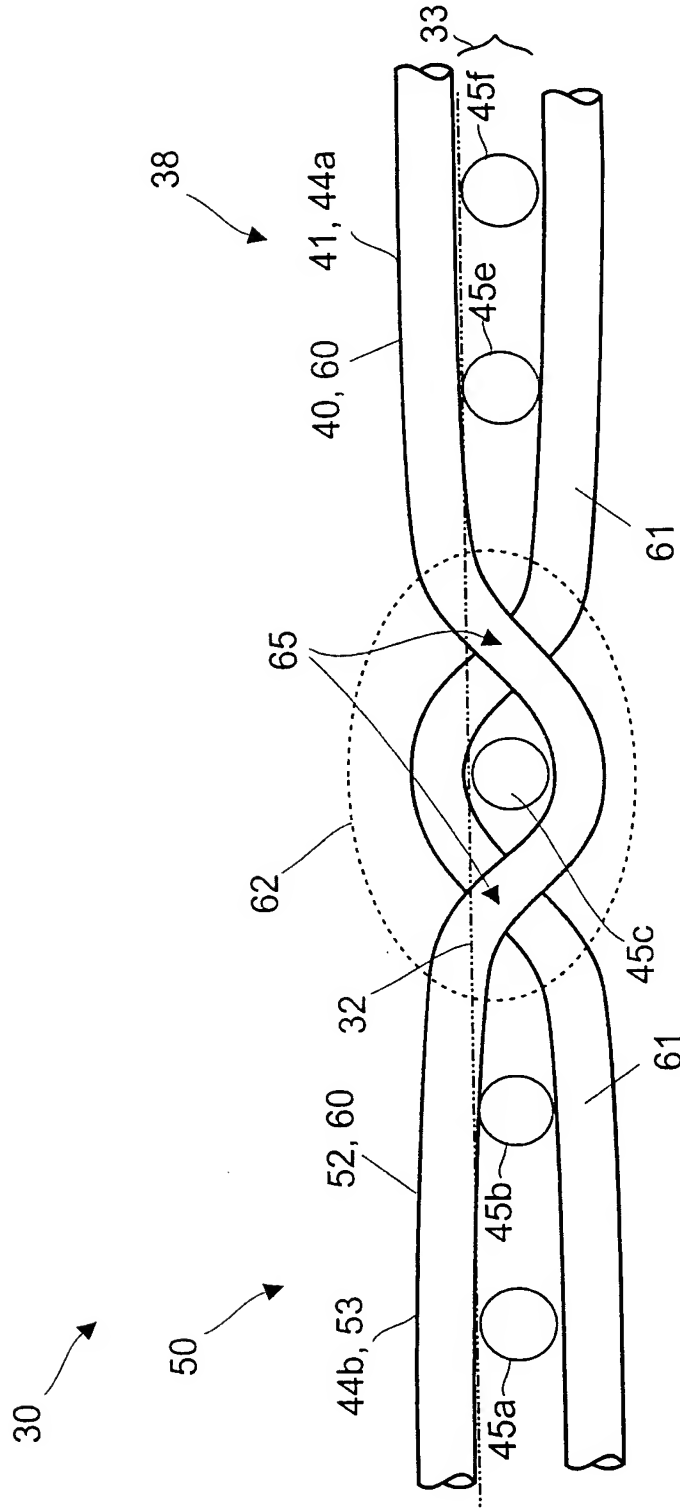


FIGURE 8

TWO "FEET" 3585T00F

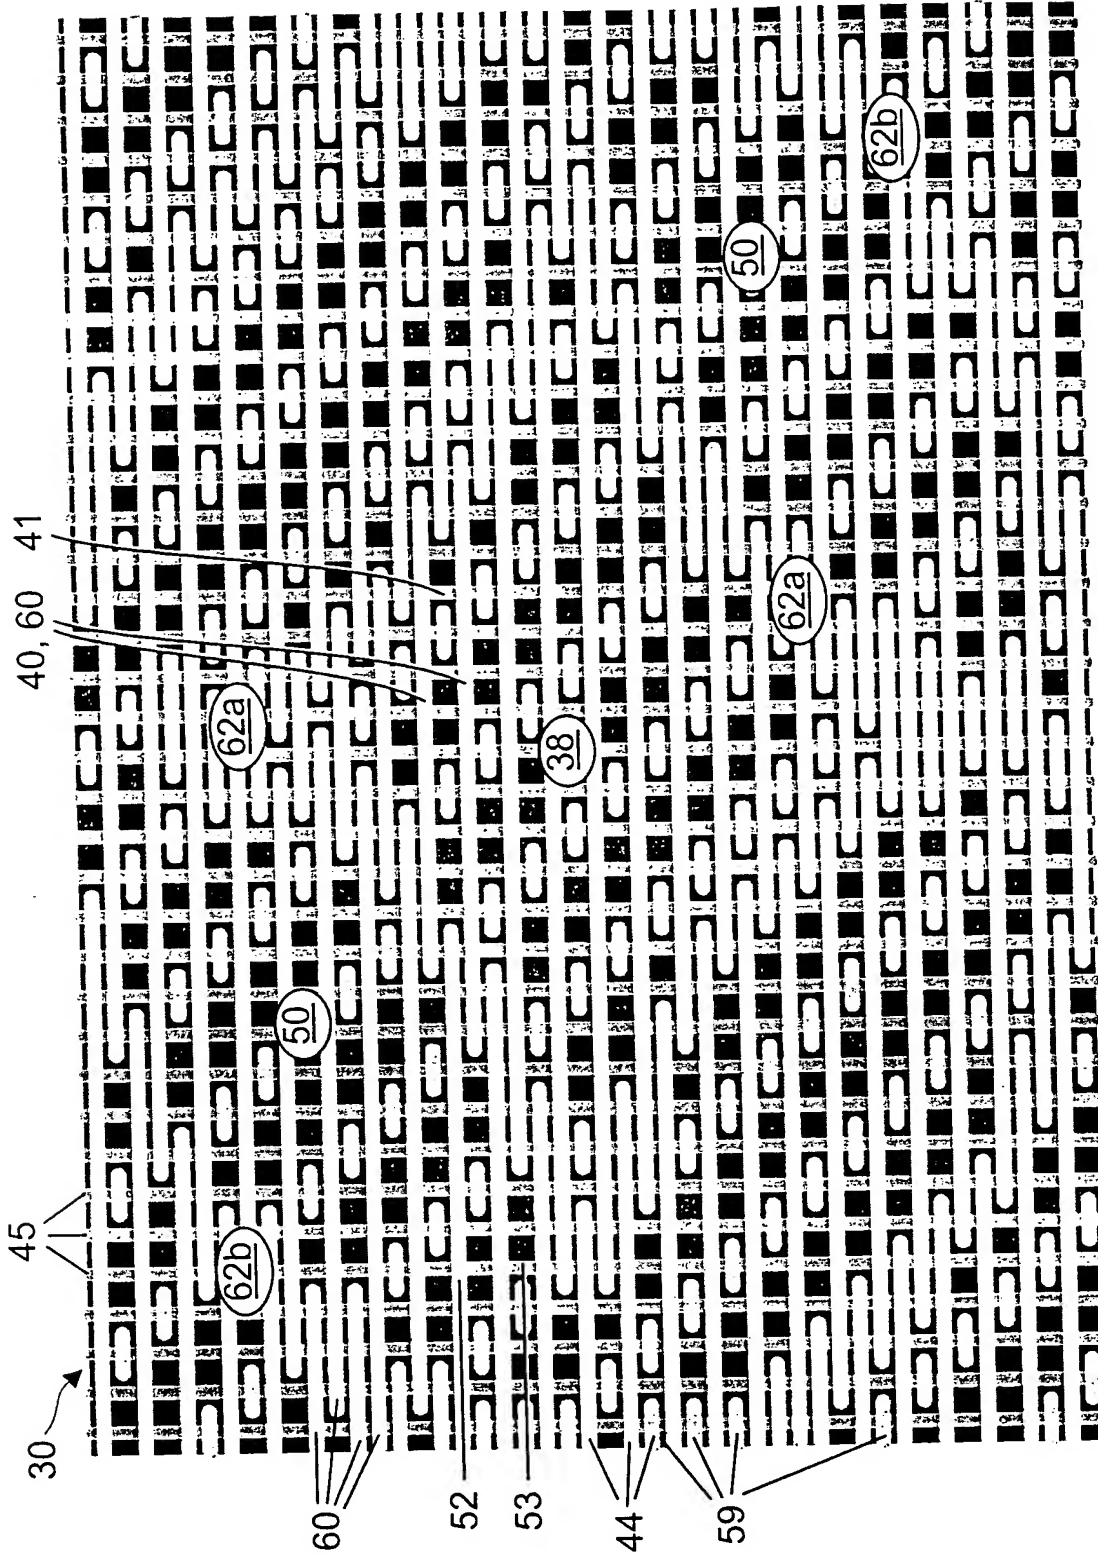



FIGURE 9

TO201T" 89851001

CADEYES Display V3.01 (D:\14293\PUTTY1.IMG)

File Log Calibration Image Processor Fiber Tech Marvels Help Clueless?

Interactive Mode: Select a function from the Command buttons

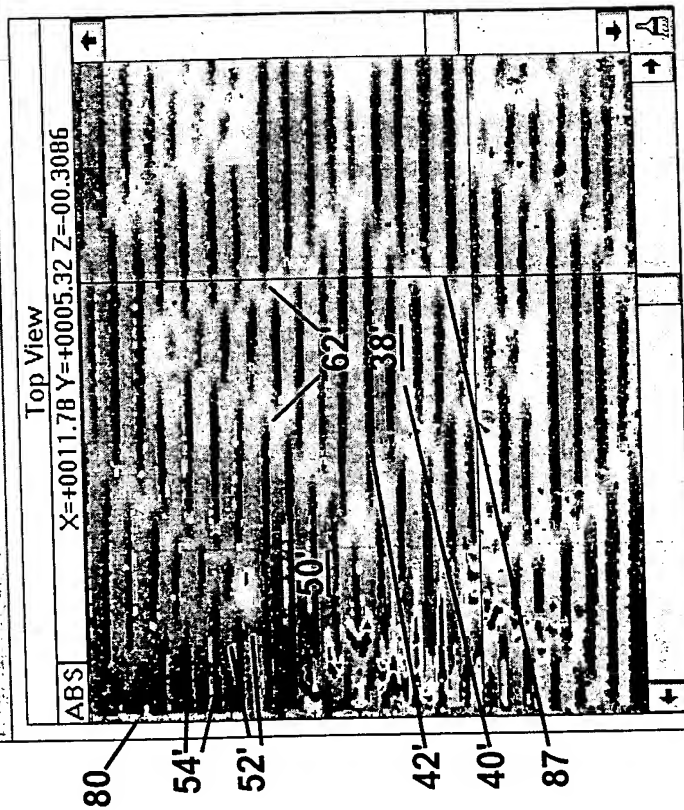

Command / Result Log

Number of points extracted = +83060.0000
PlaneFit points = +83060.0000
Xslope = +00.0016
Yslope = +00.0258
Offset = +00.0540
Ra = +00.2047
Flatness = +01.6521

Commands

MAG.	OFFS.
Auto Scale	
-0.8813	
-0.5313	
-0.1812	
+0.1689	
+0.5190	
+0.8691	
+1.2191	

Zoom In	Palette
Zoom Out	3-D View
512 x 512	Fix Data
Plane Fit	Sphere Fit
Quad Fit	Average
AcquireData	AreaAve
Application	

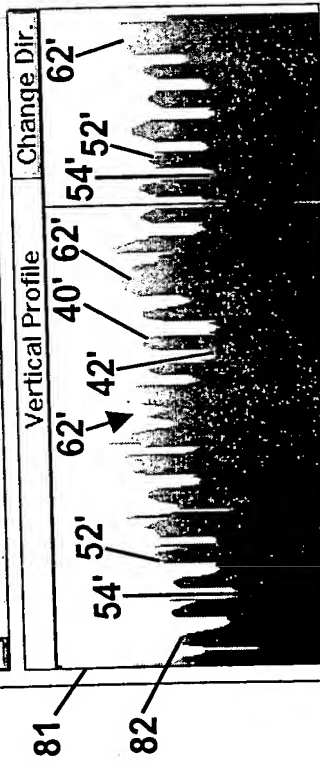


FIGURE 10.

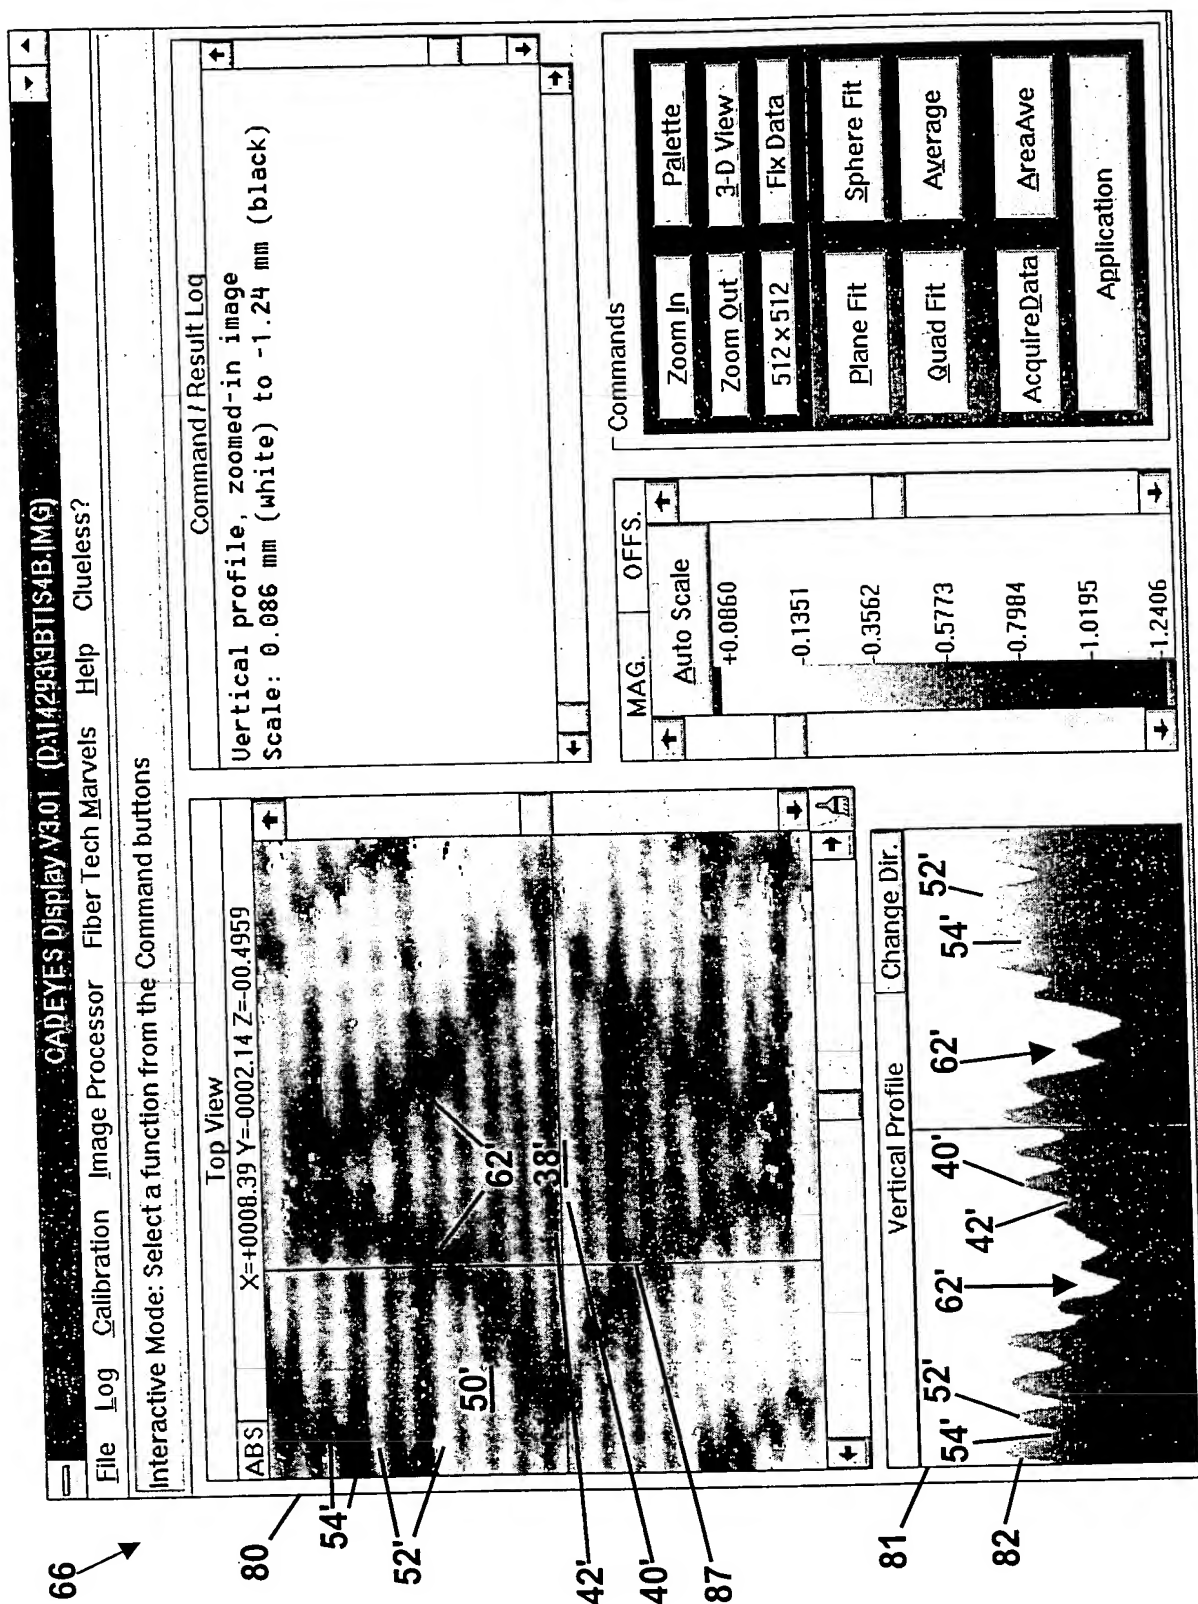



FIGURE 11.



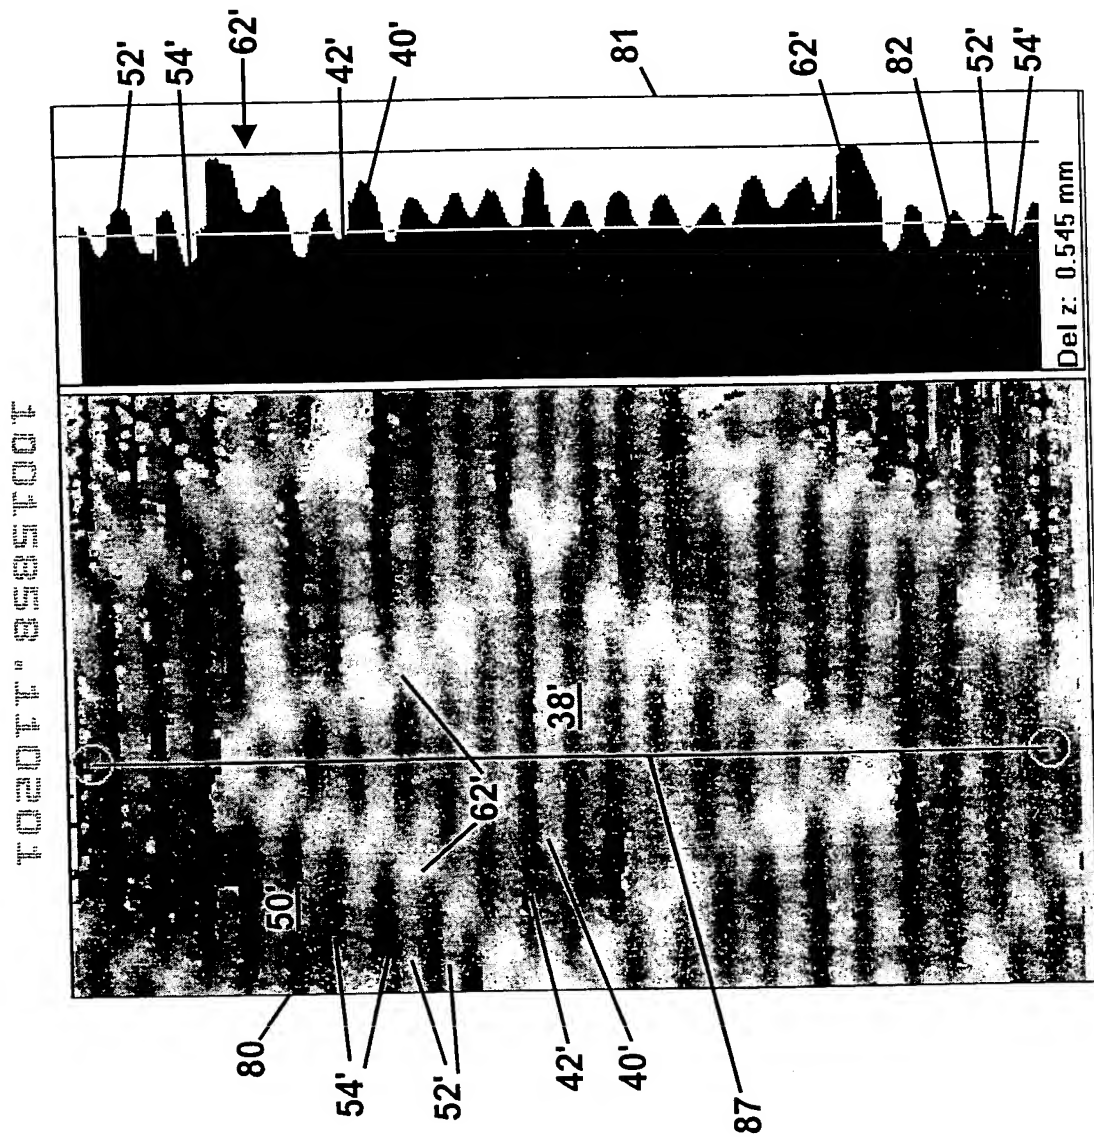


FIGURE 13.

FOOT" 3585FOOT

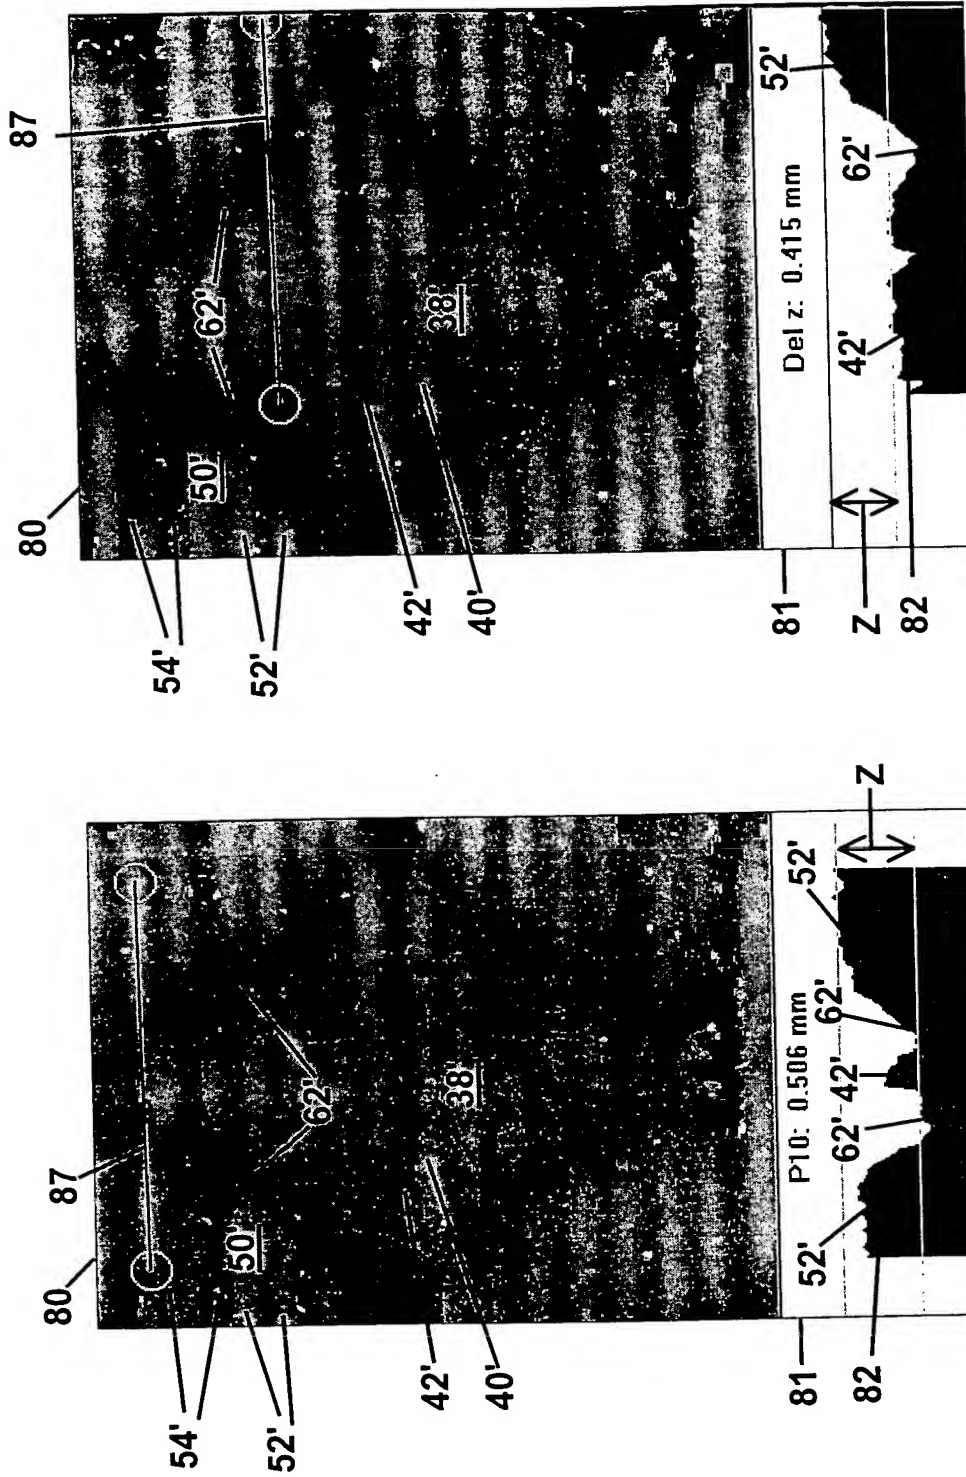


FIGURE 15.

FIGURE 14.

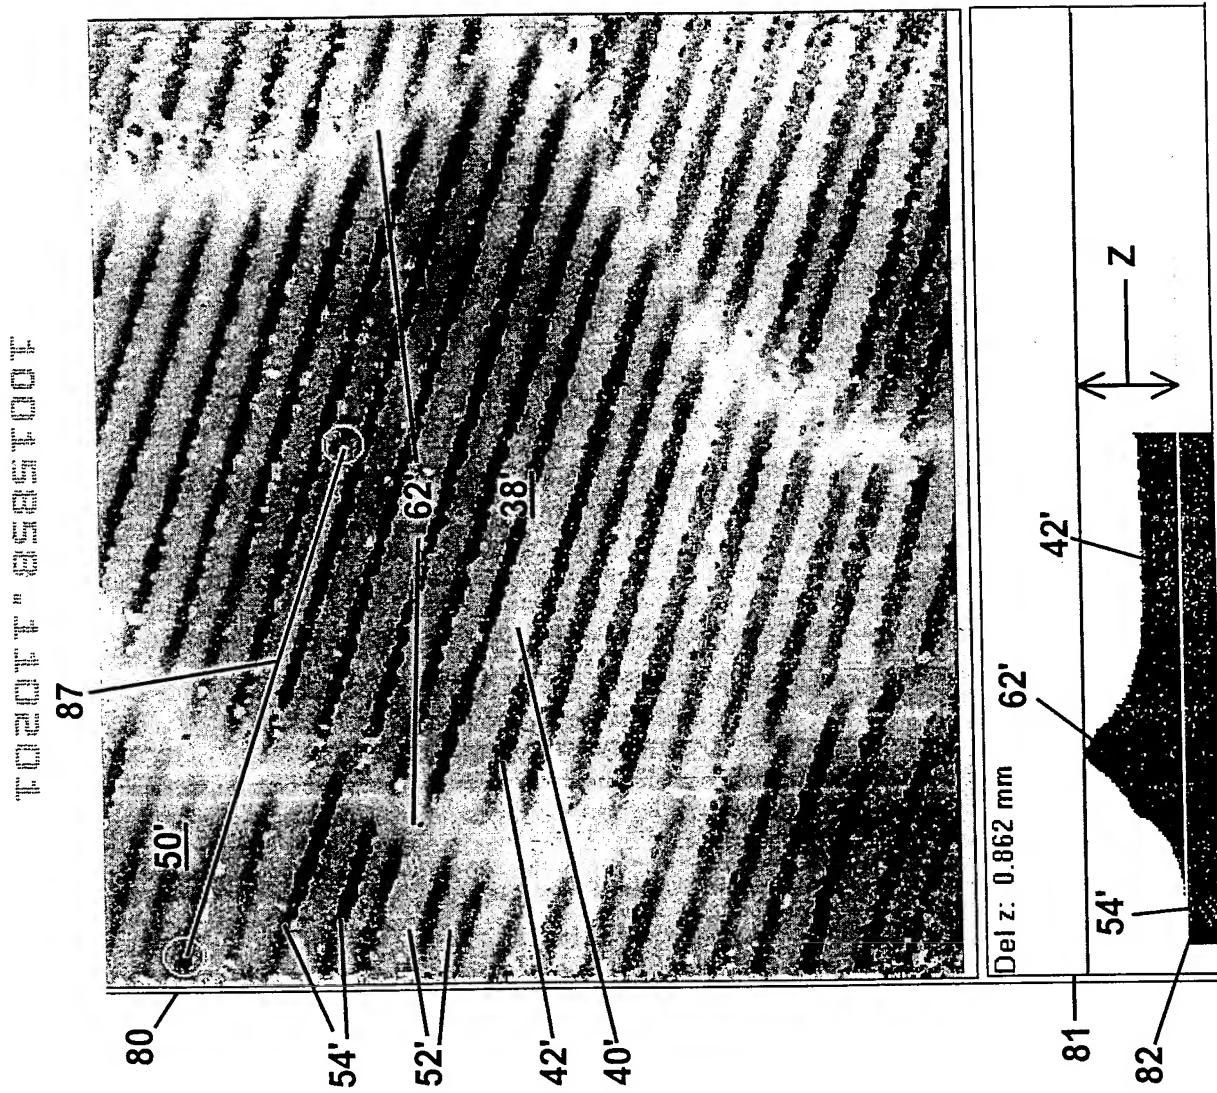


FIGURE 16.

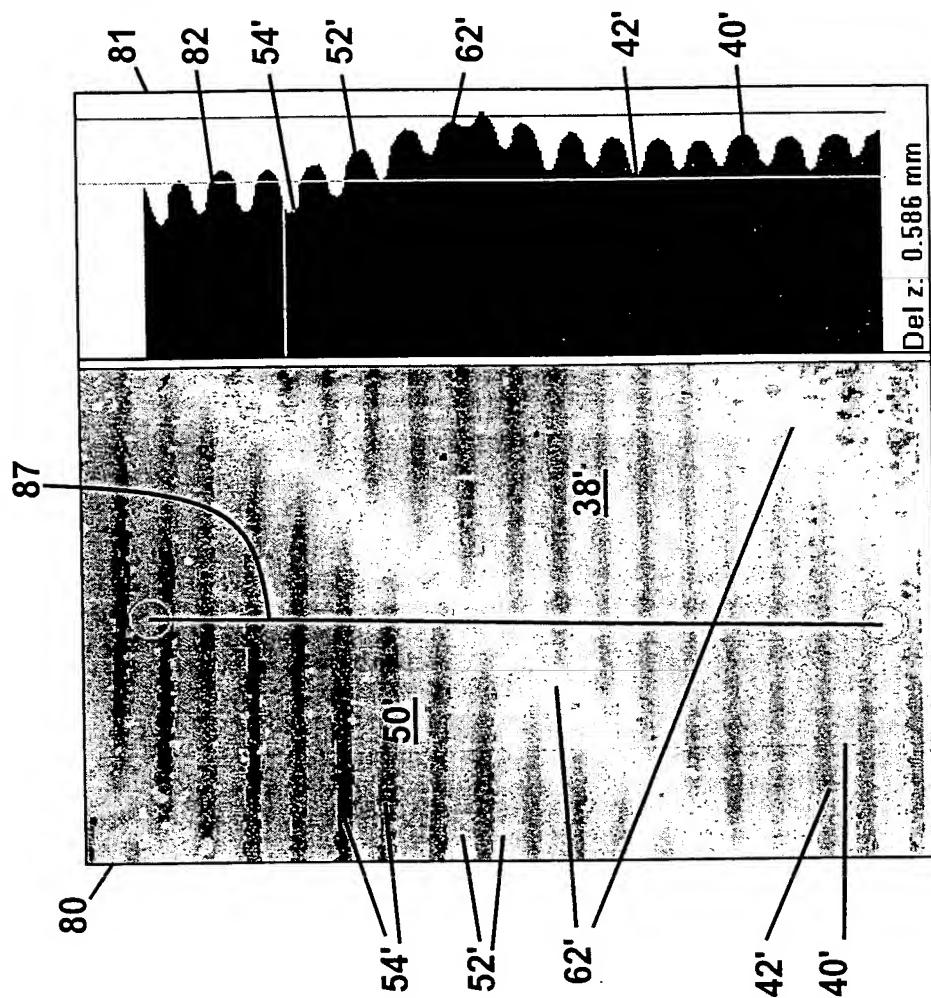


FIGURE 17.

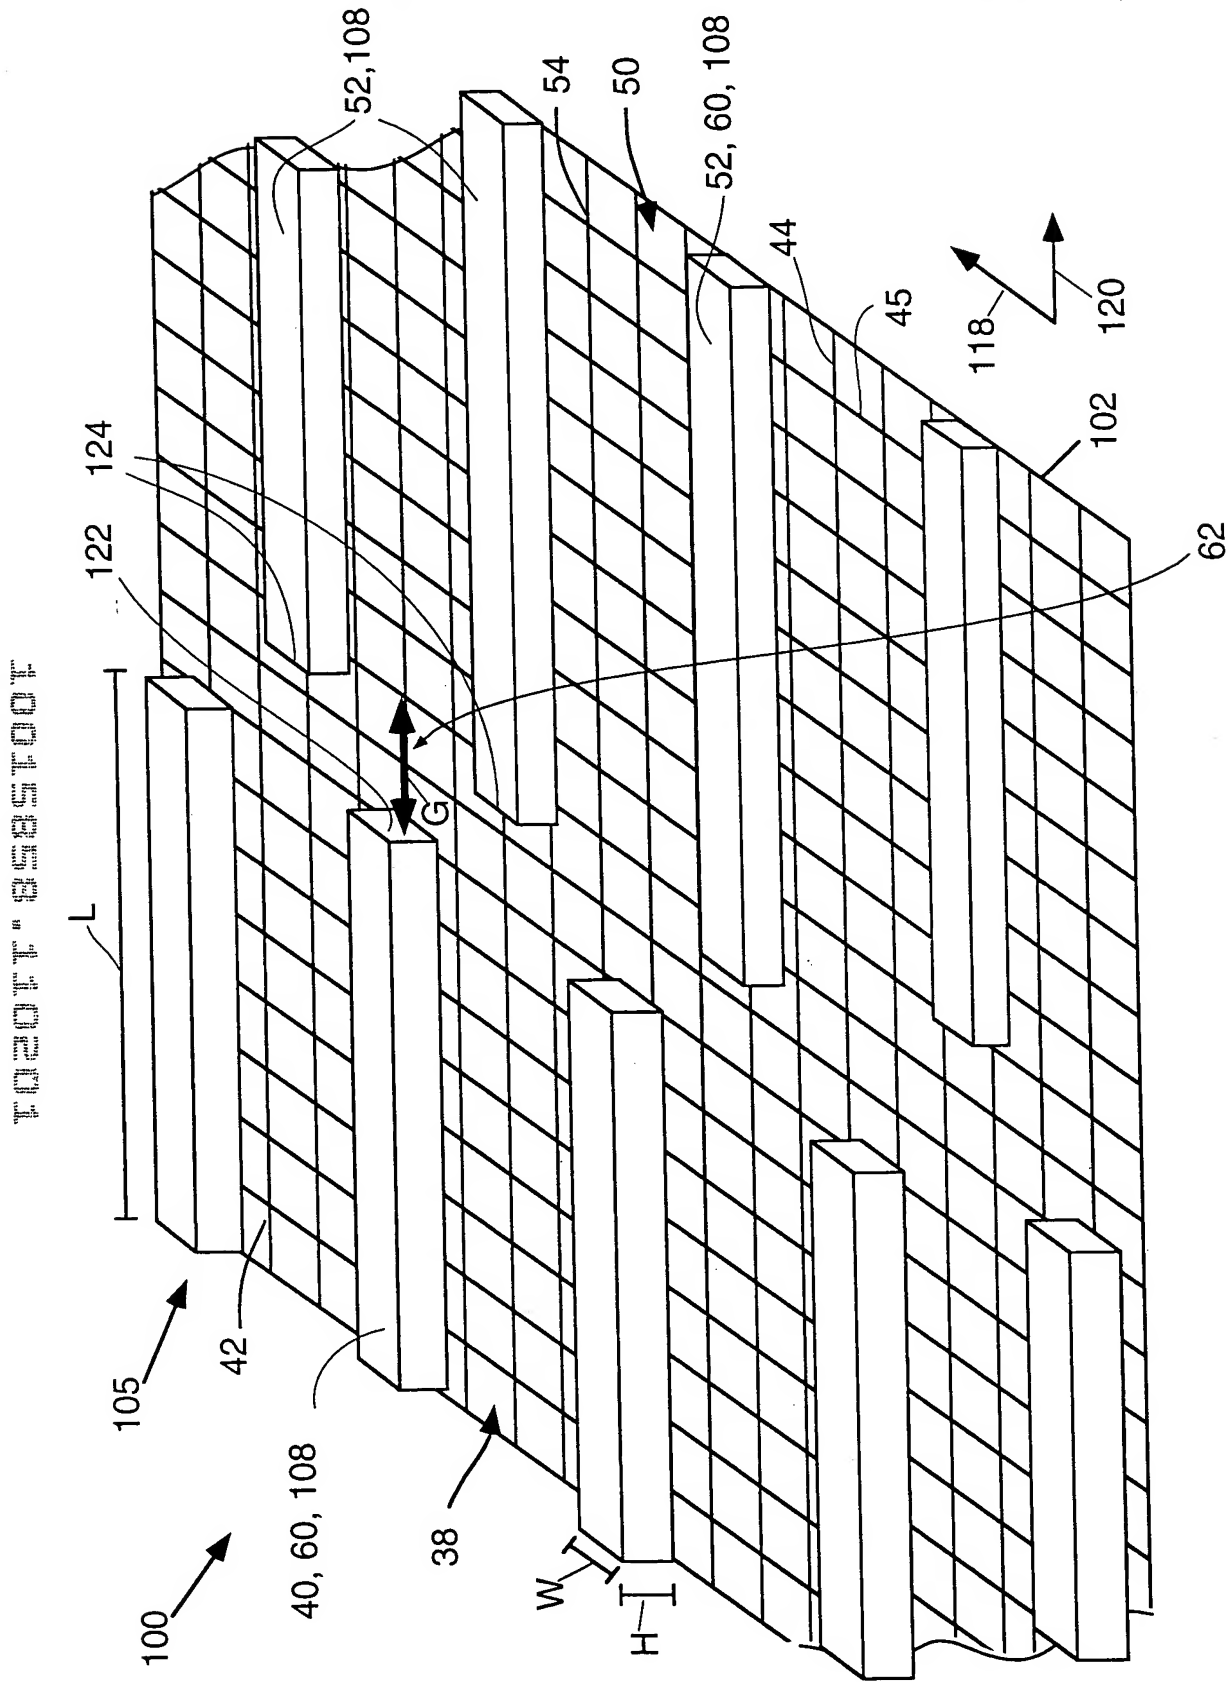


FIGURE 18



FIGURE 19

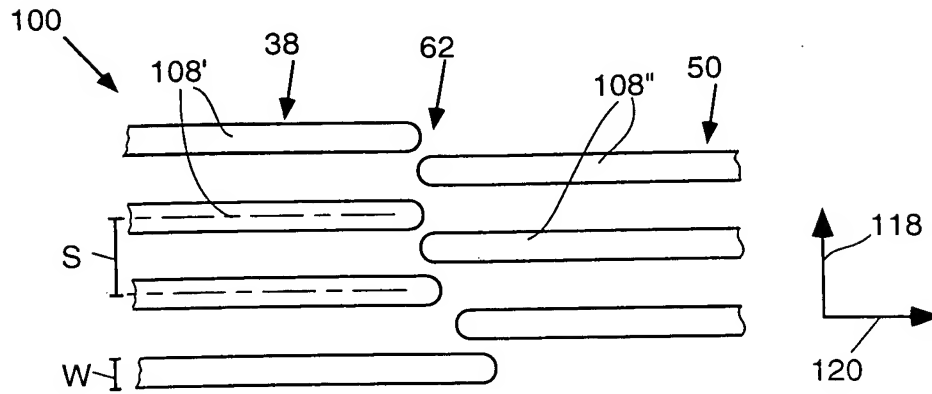


FIGURE 20

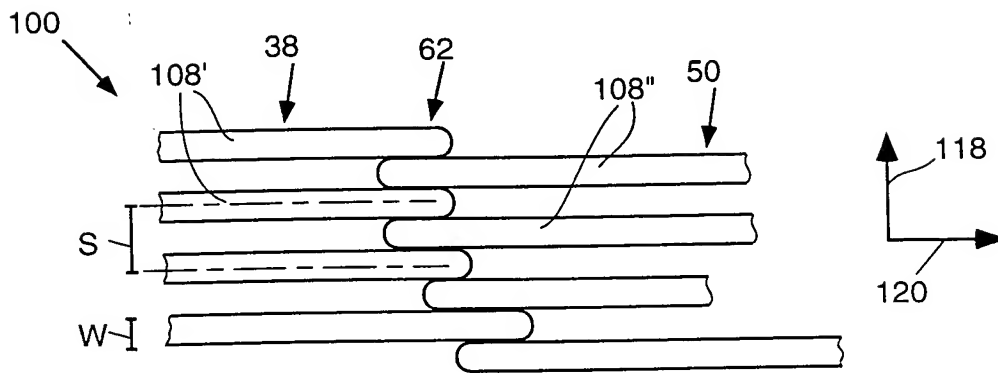


FIGURE 21

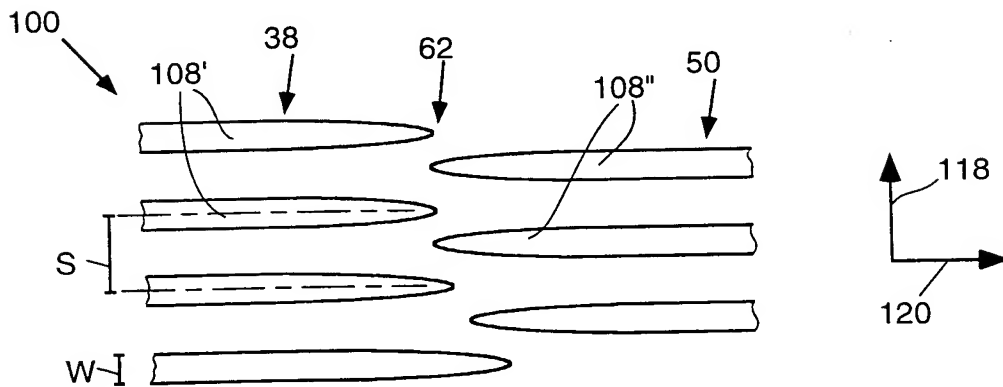


FIGURE 22

10015858 " 110201

FOOTNOTES

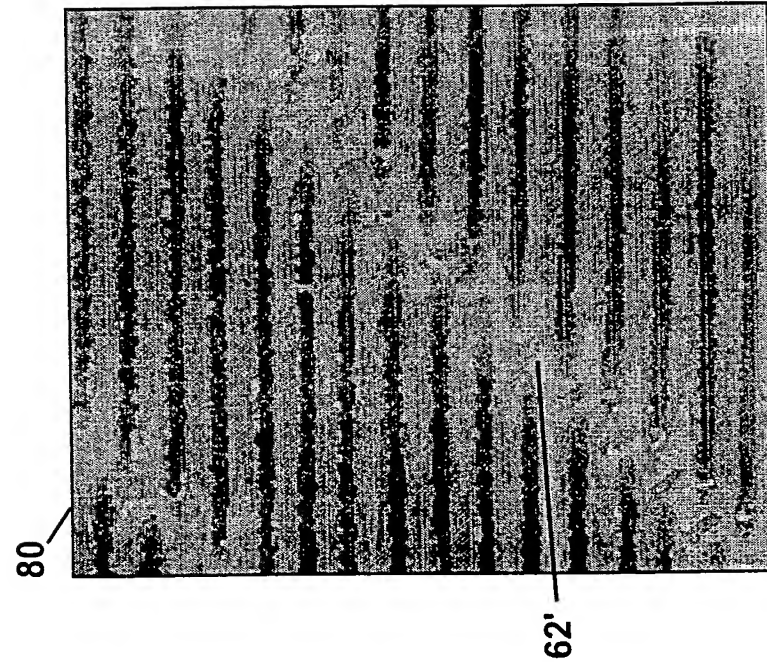


FIGURE 23.

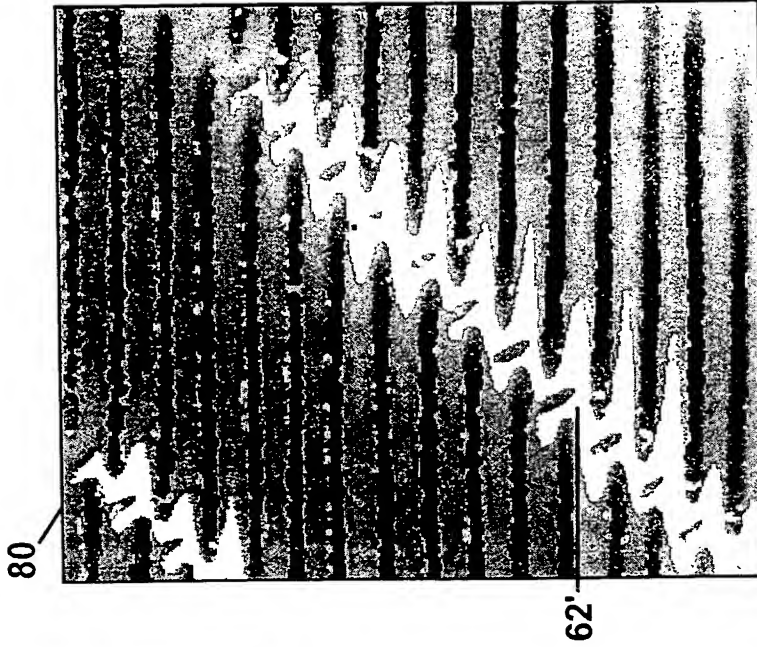


FIGURE 24.

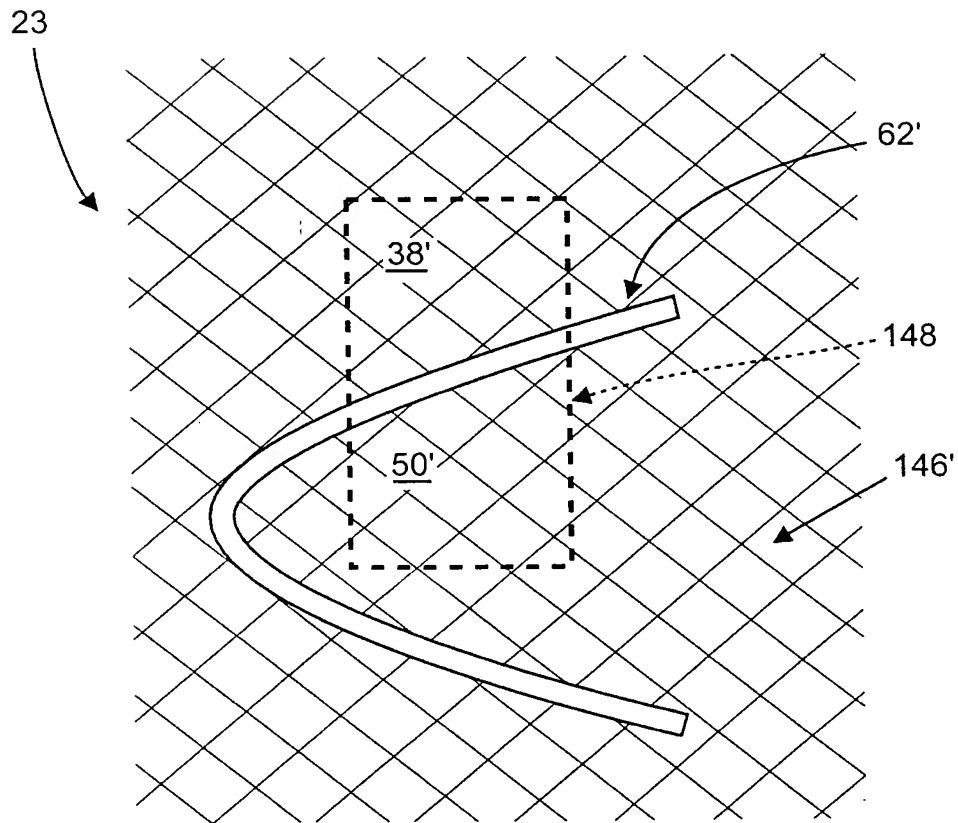


FIGURE 25

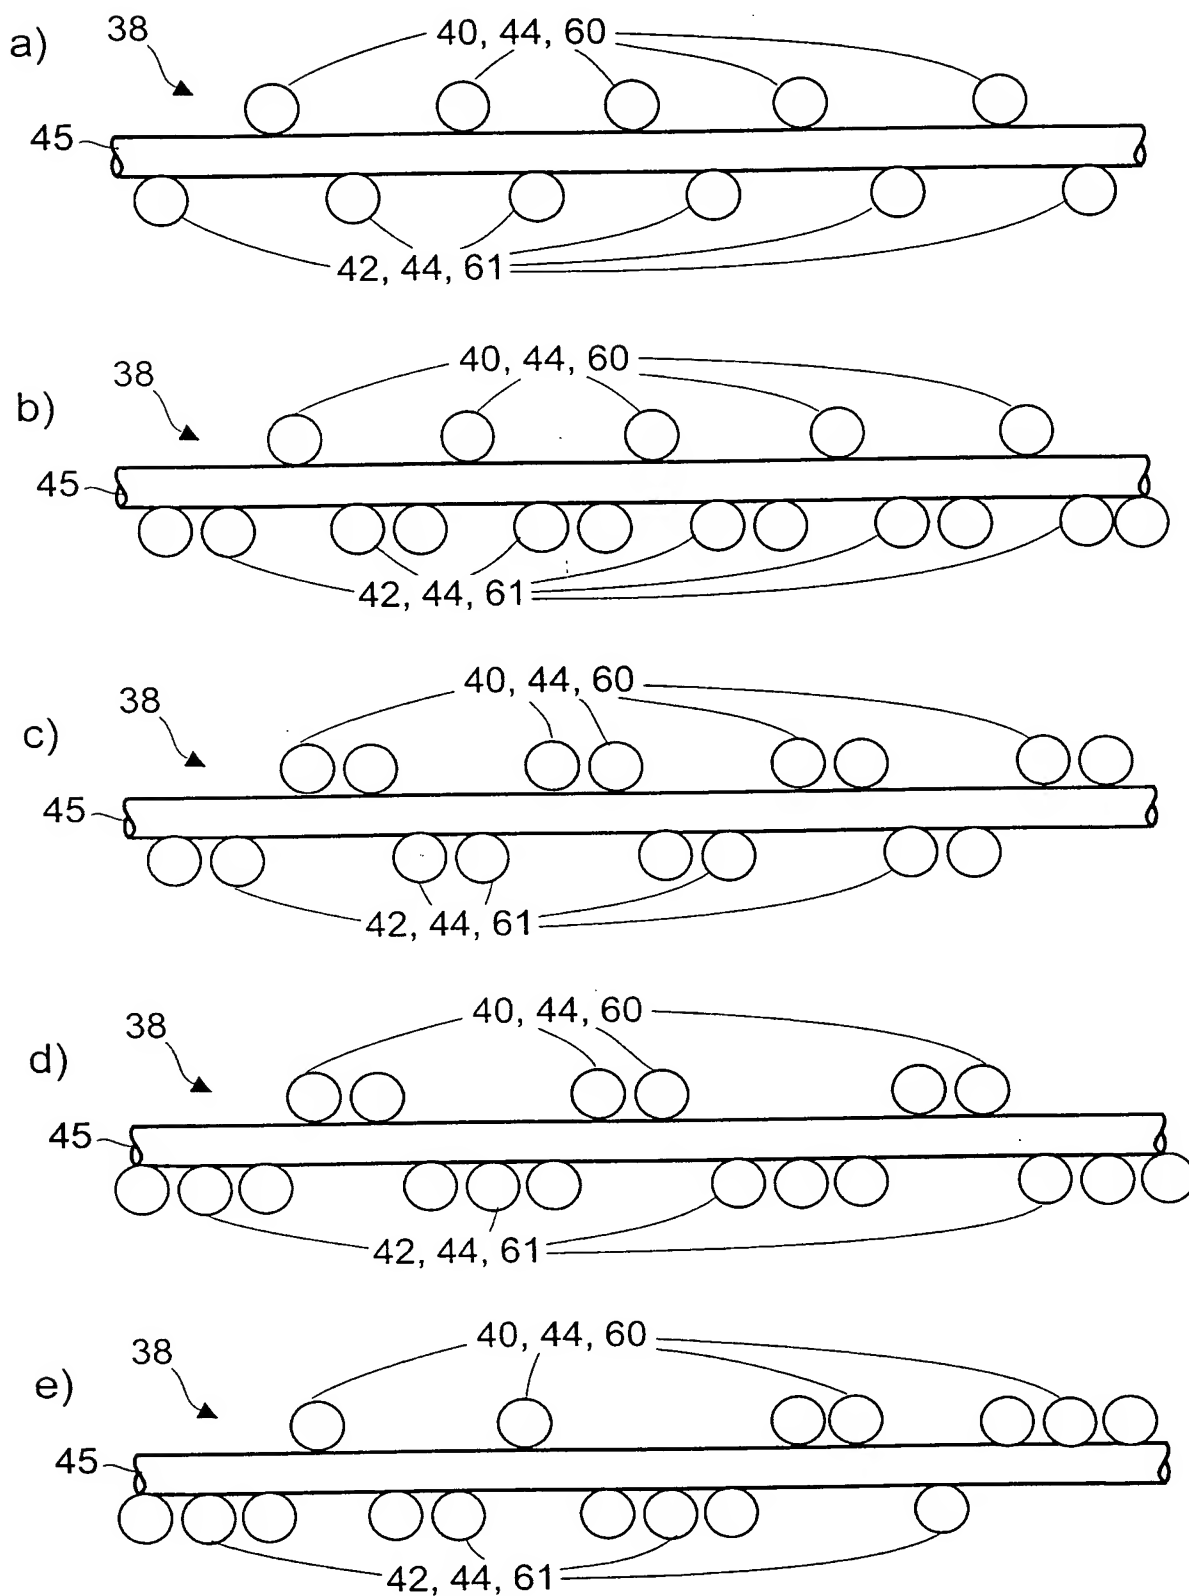


FIGURE 26

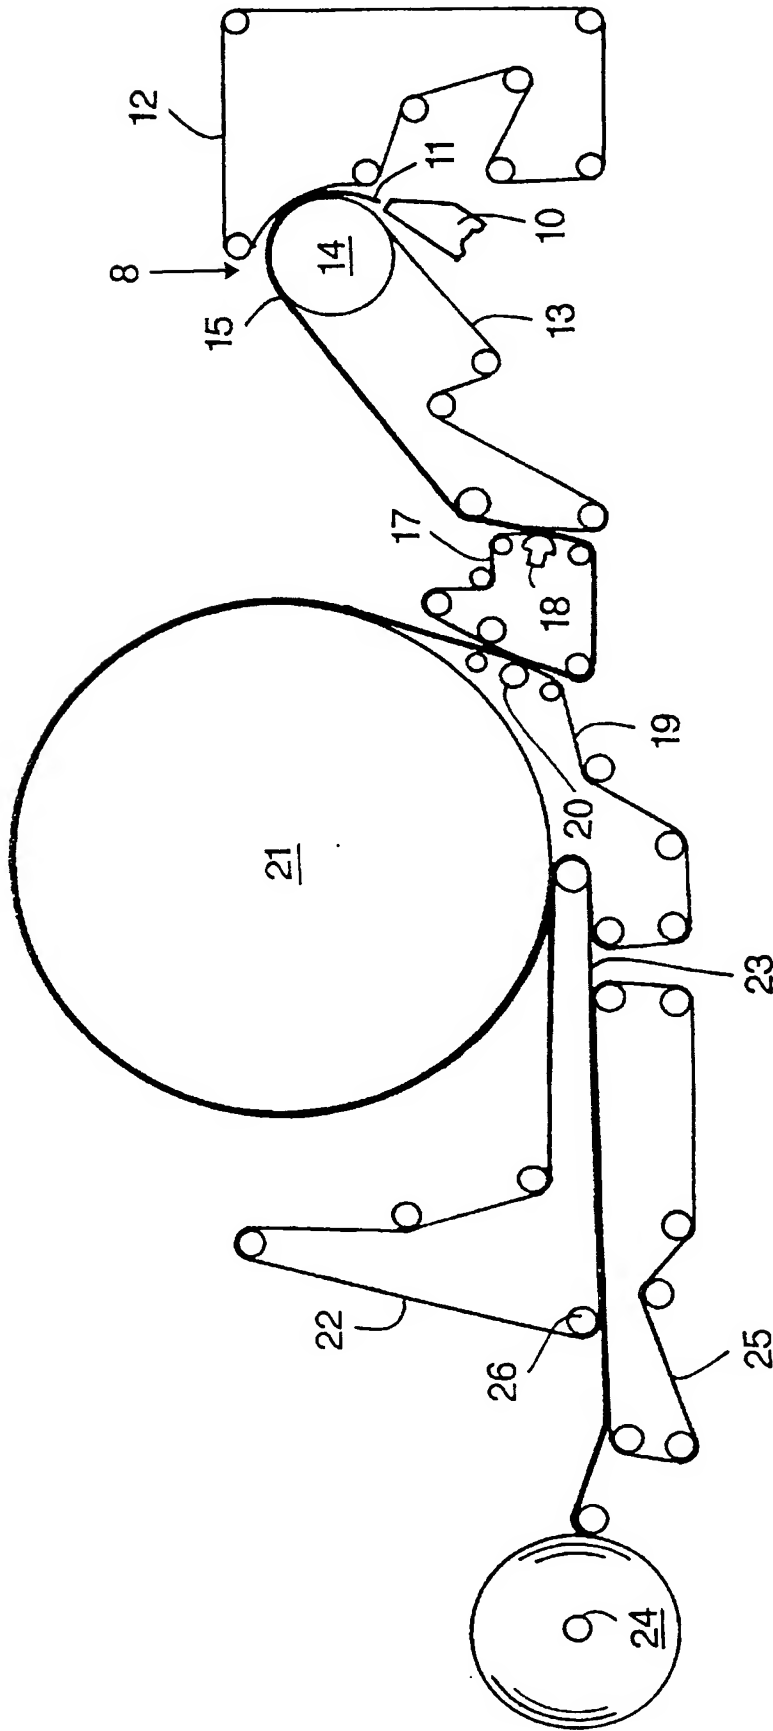


FIGURE 27

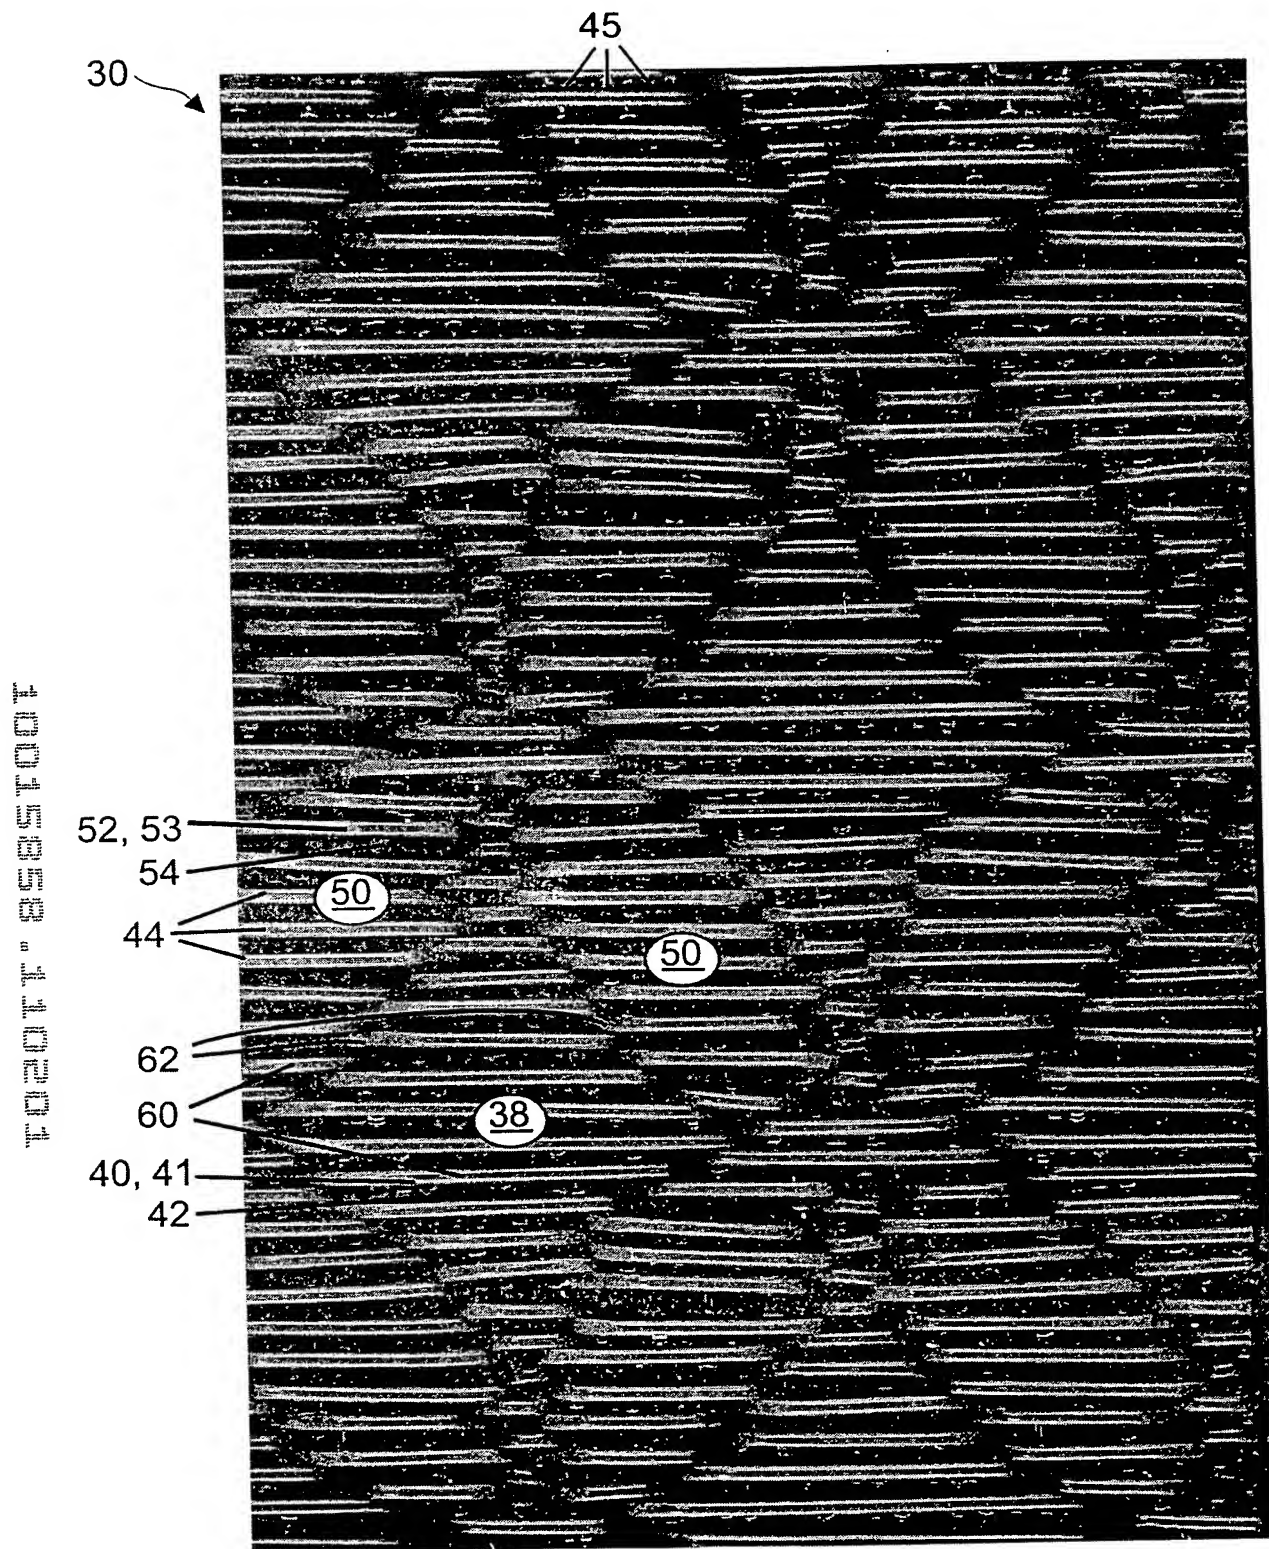


FIGURE 28

10015858 "110201

23

52'
54'
62'
40'
42'

50'

50'

38'

FIGURE 29

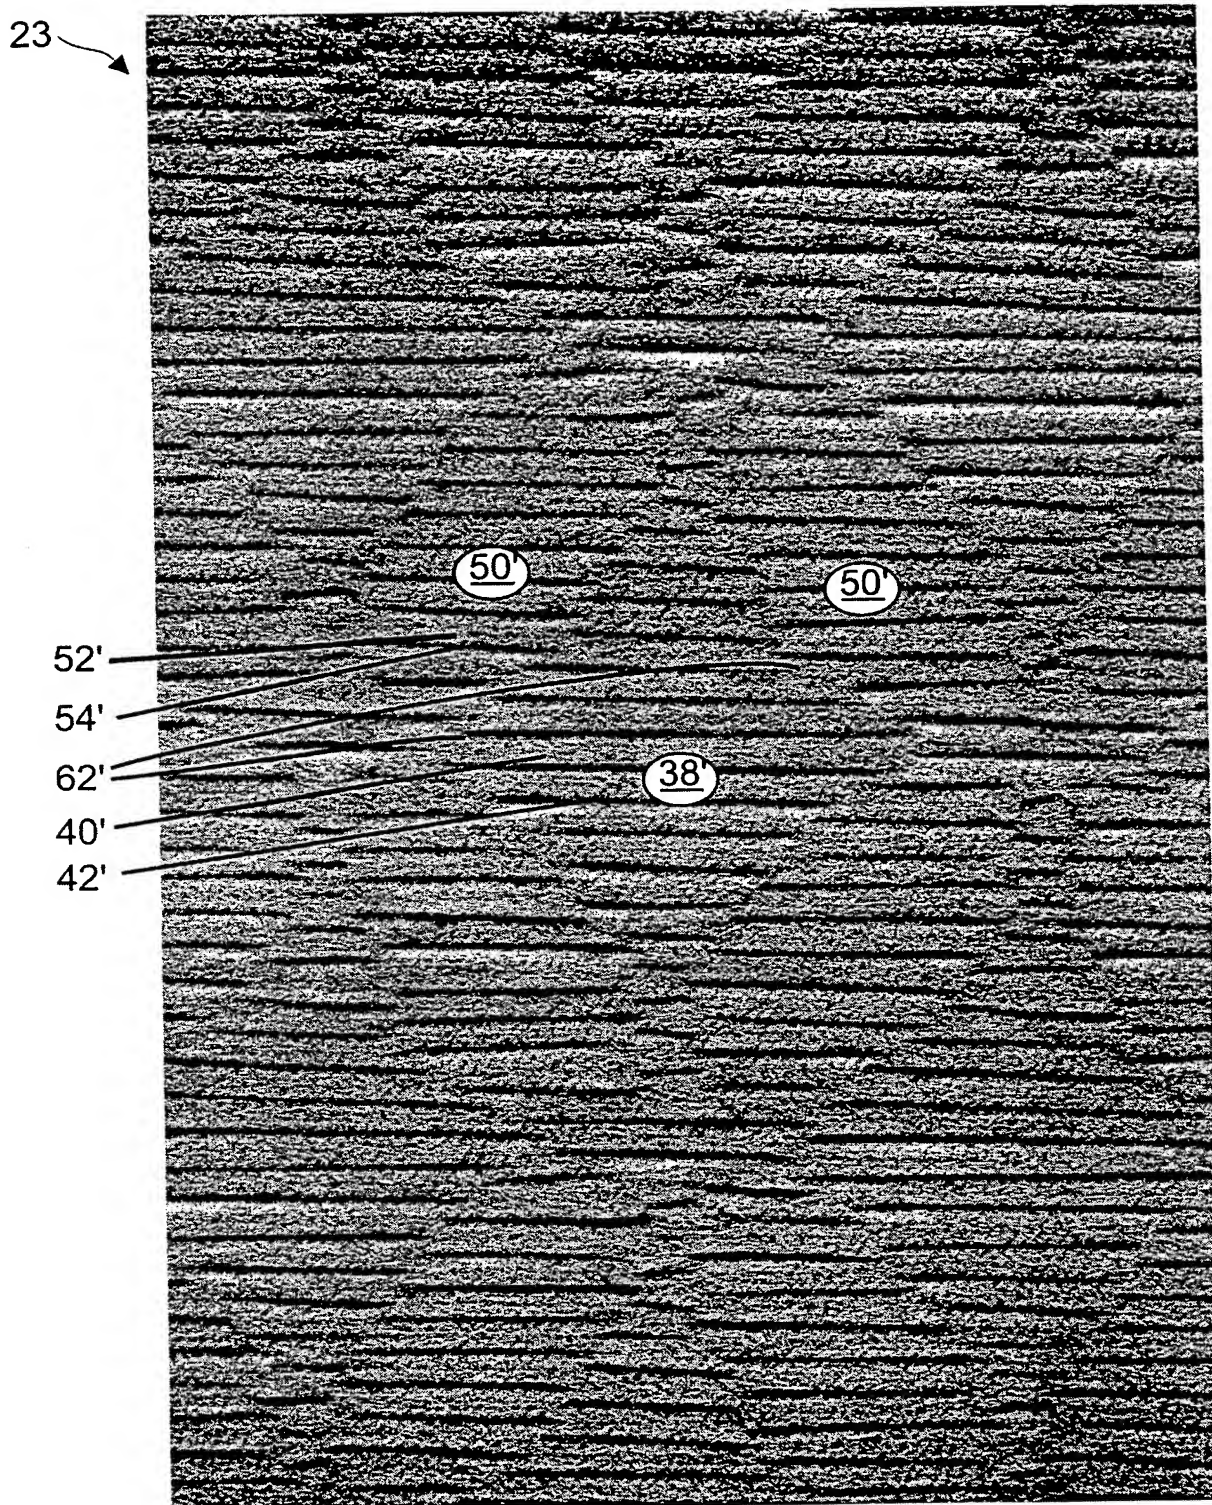


FIGURE 30